


exo

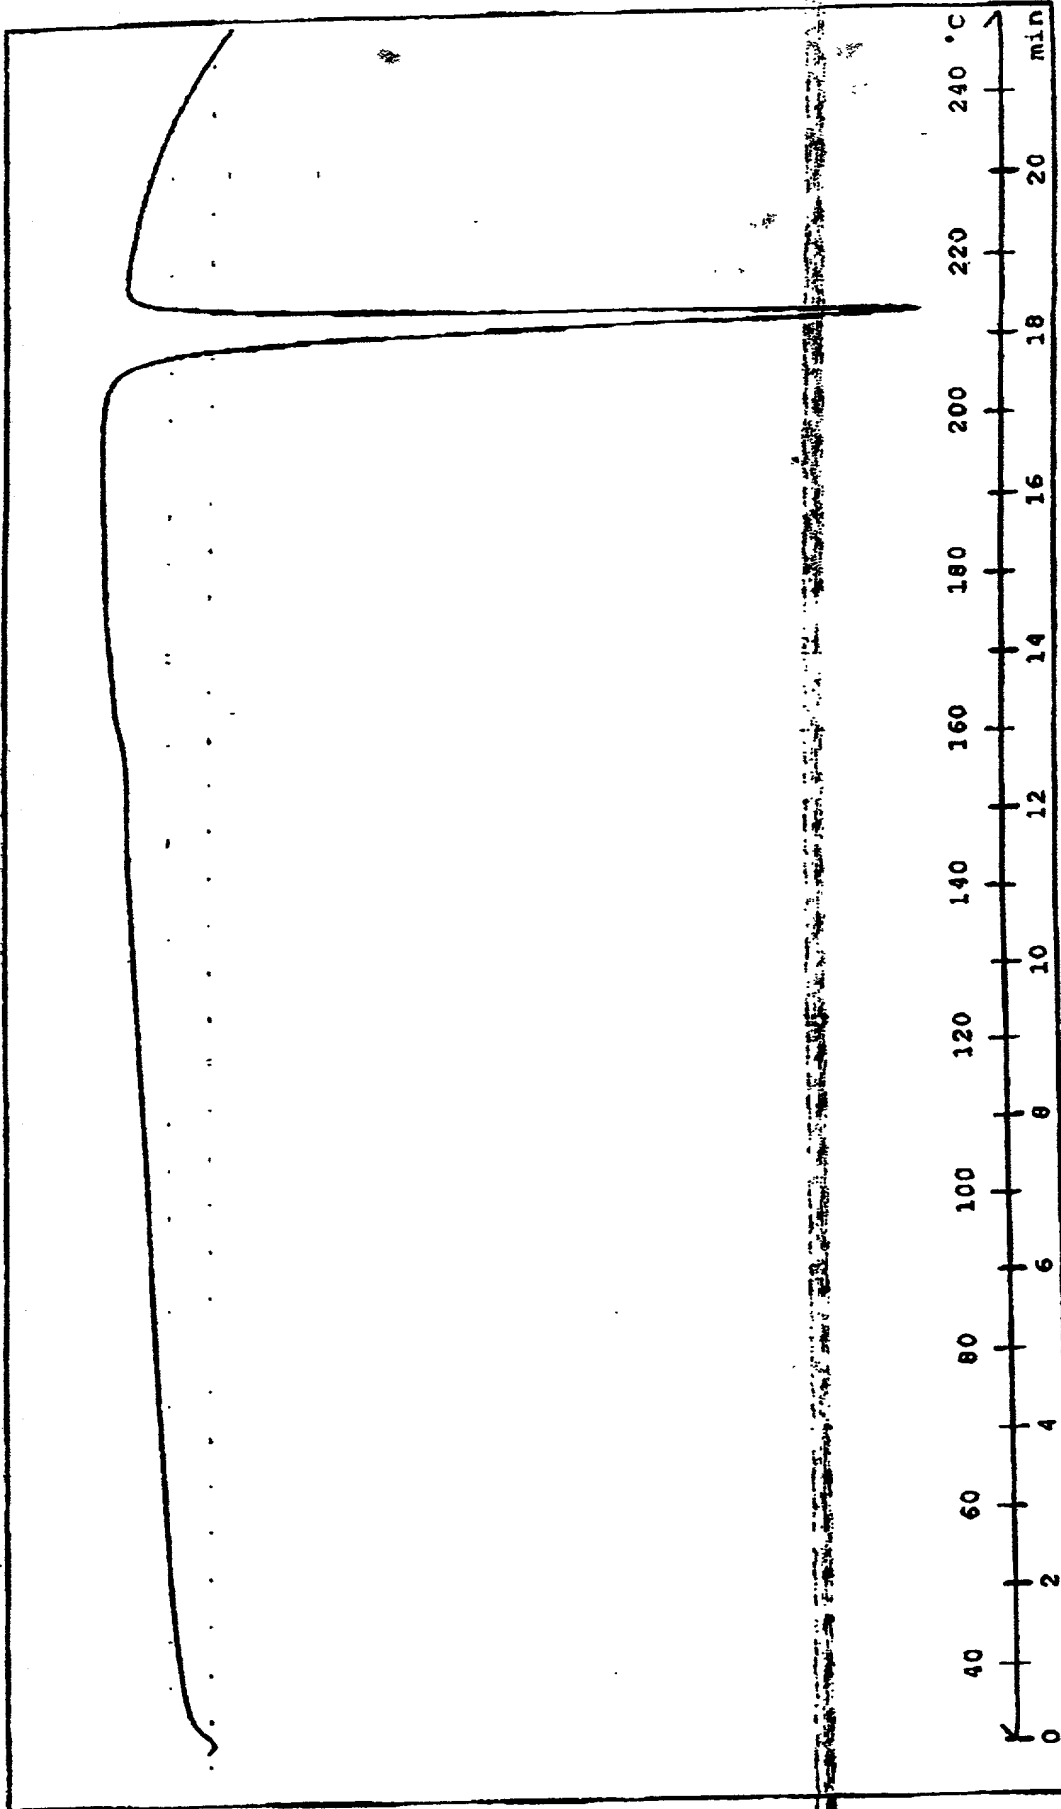

Physical R&D Teva: Shlomo

METTTLER TOLEDO STAR System

Figure 1

TEXT 340000


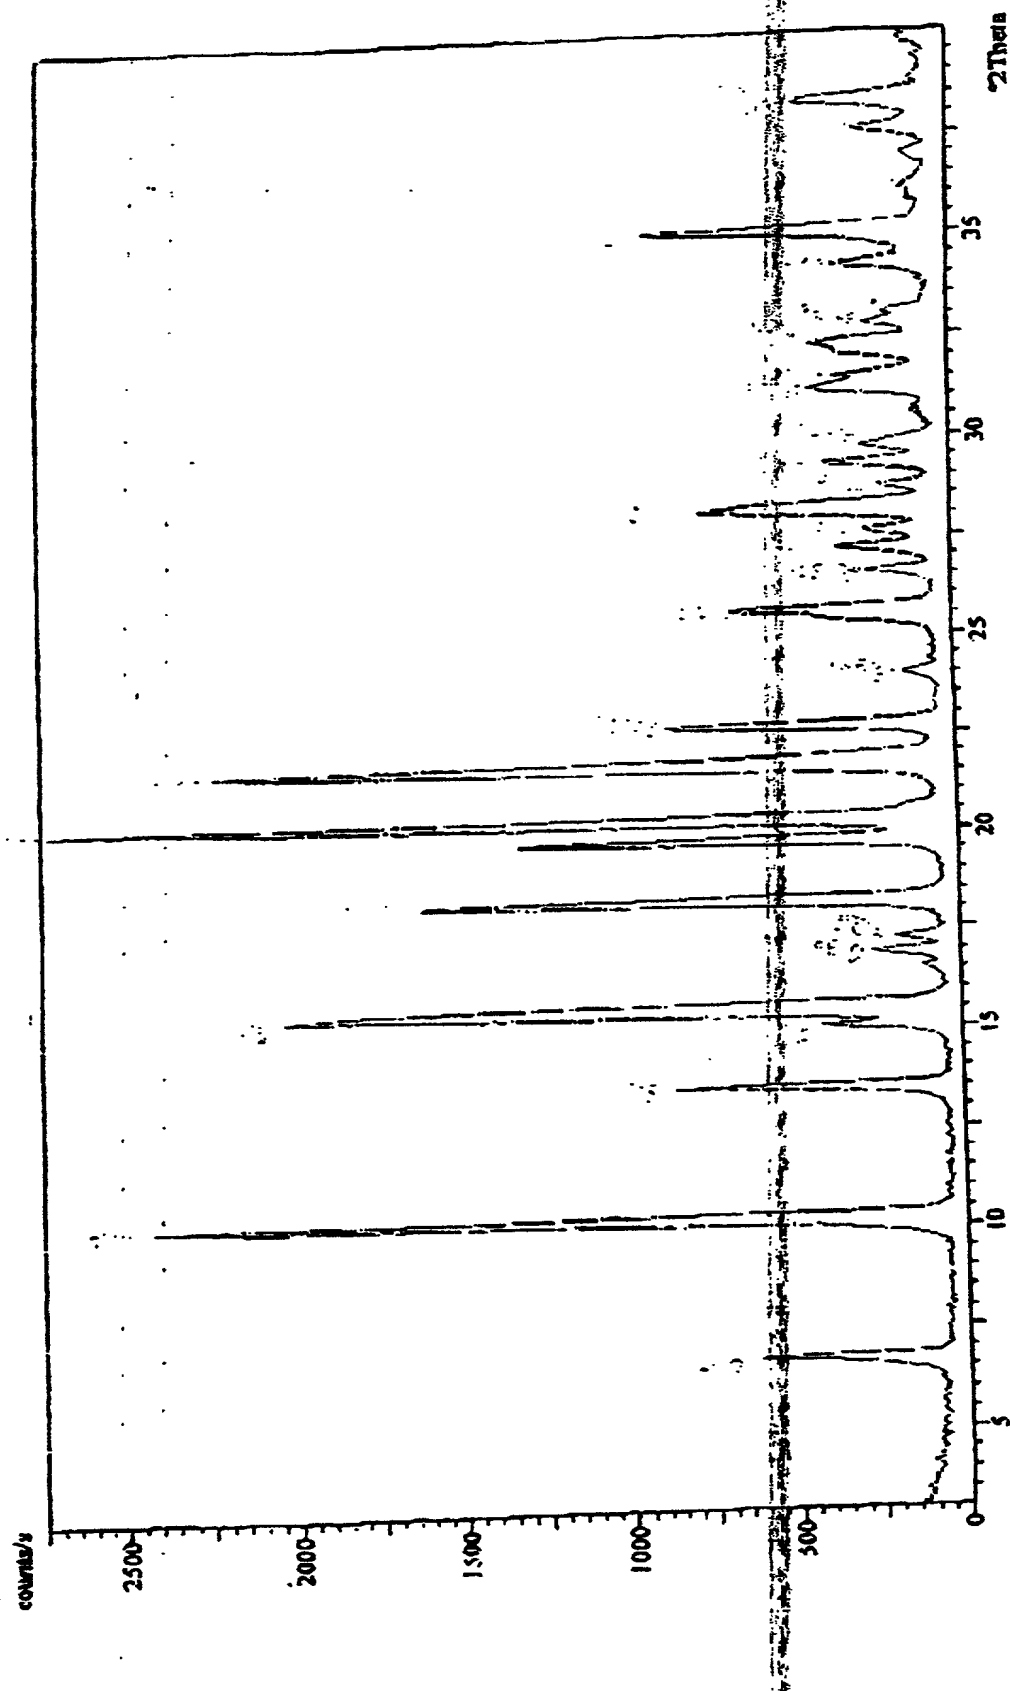


Figure 2

exo

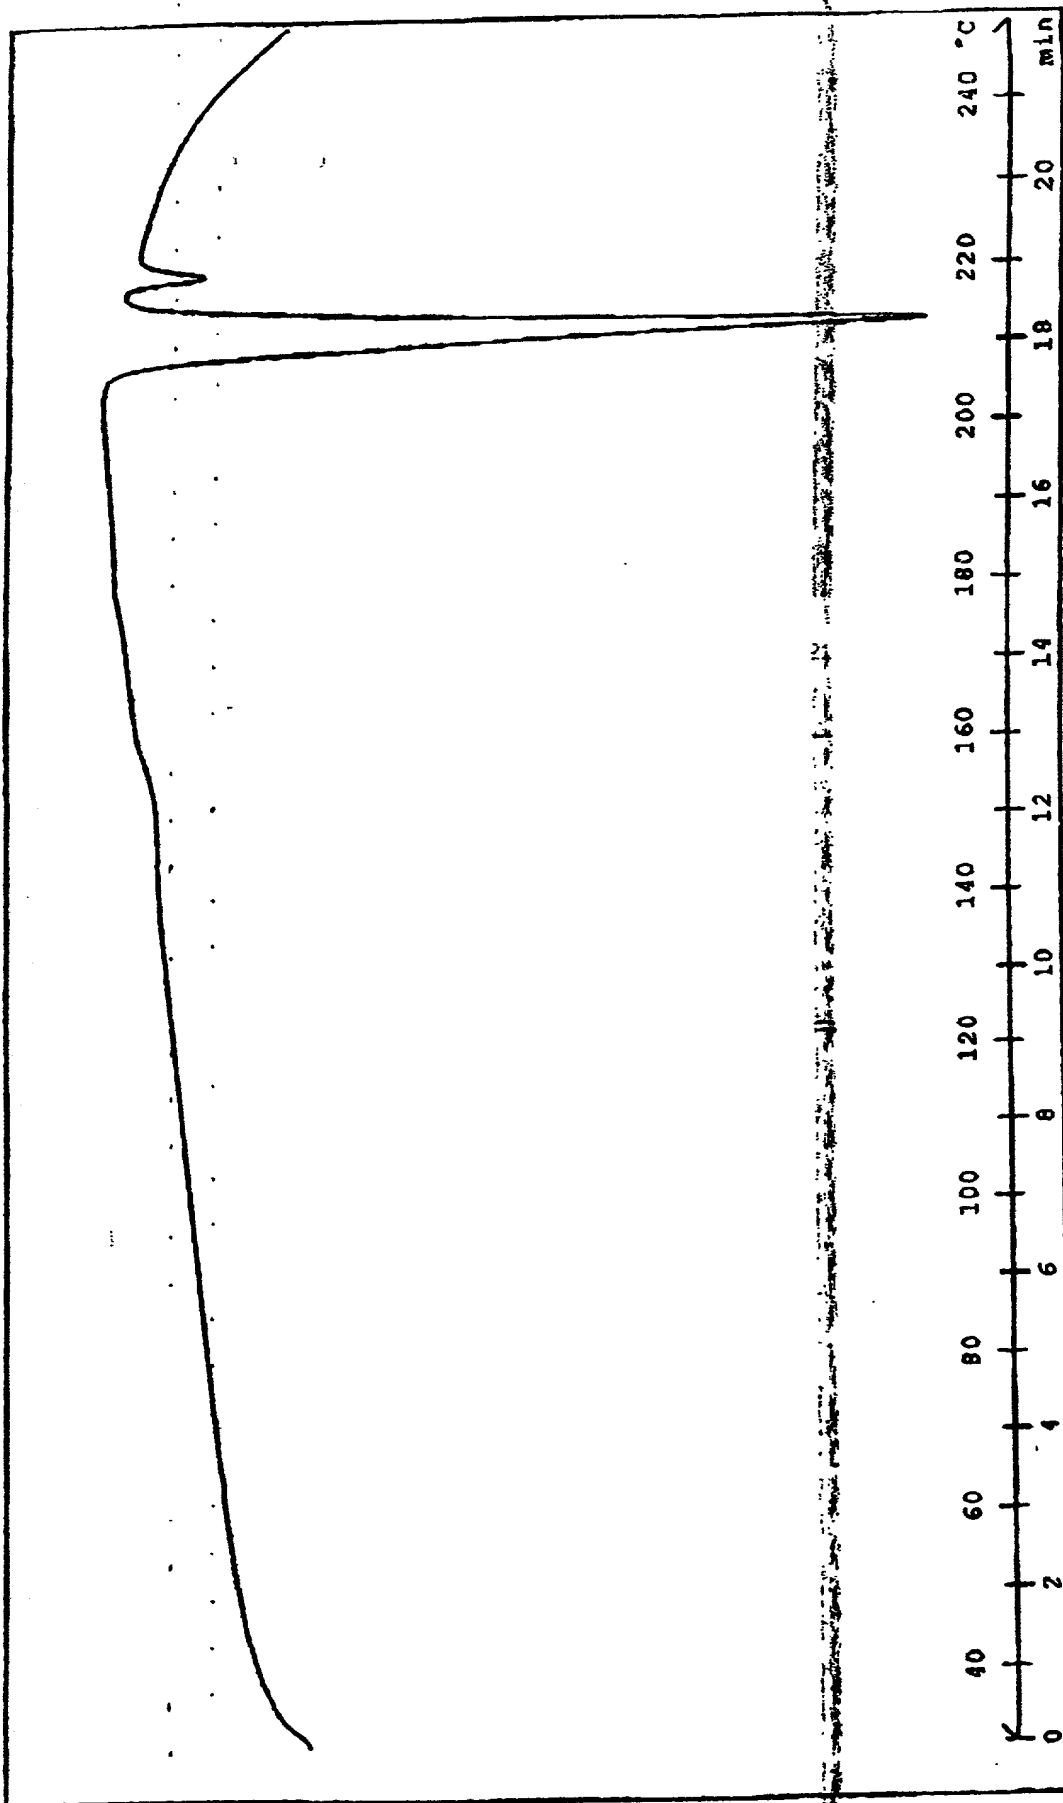

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR® System

Figure 3


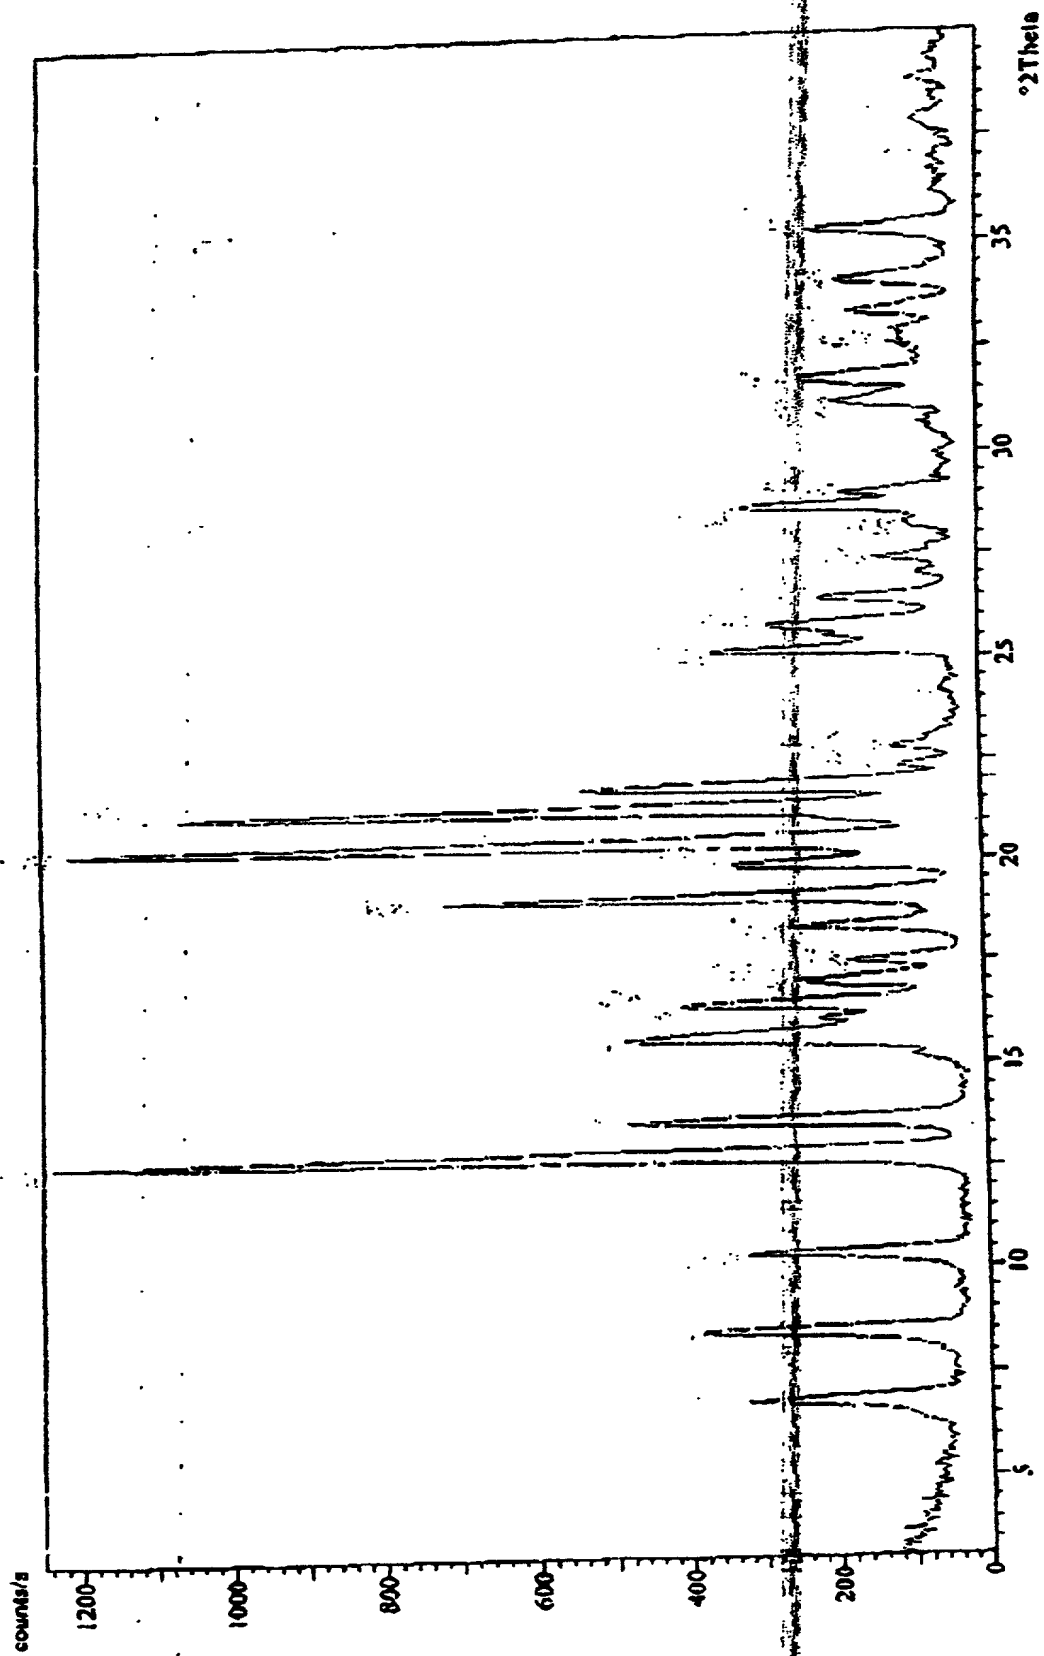


Figure 4

exo

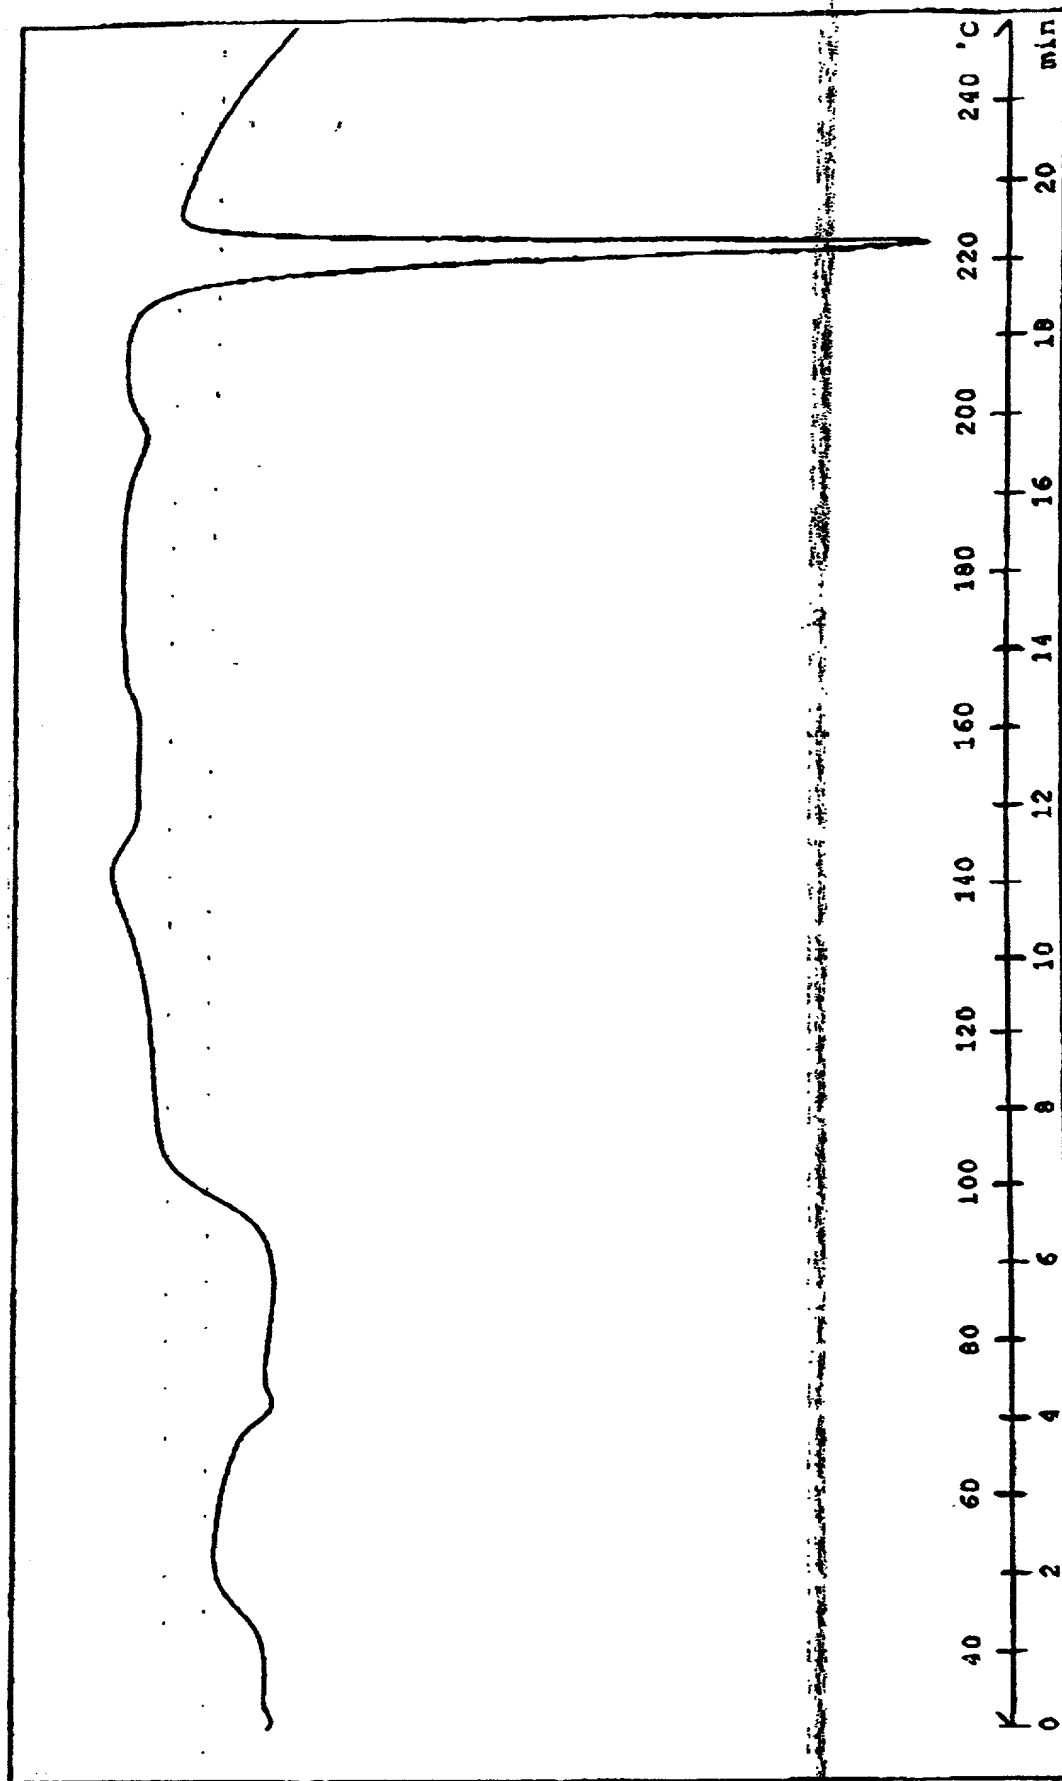

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR System

Figure 5

TOOT 340000

III

TOTAL P.03


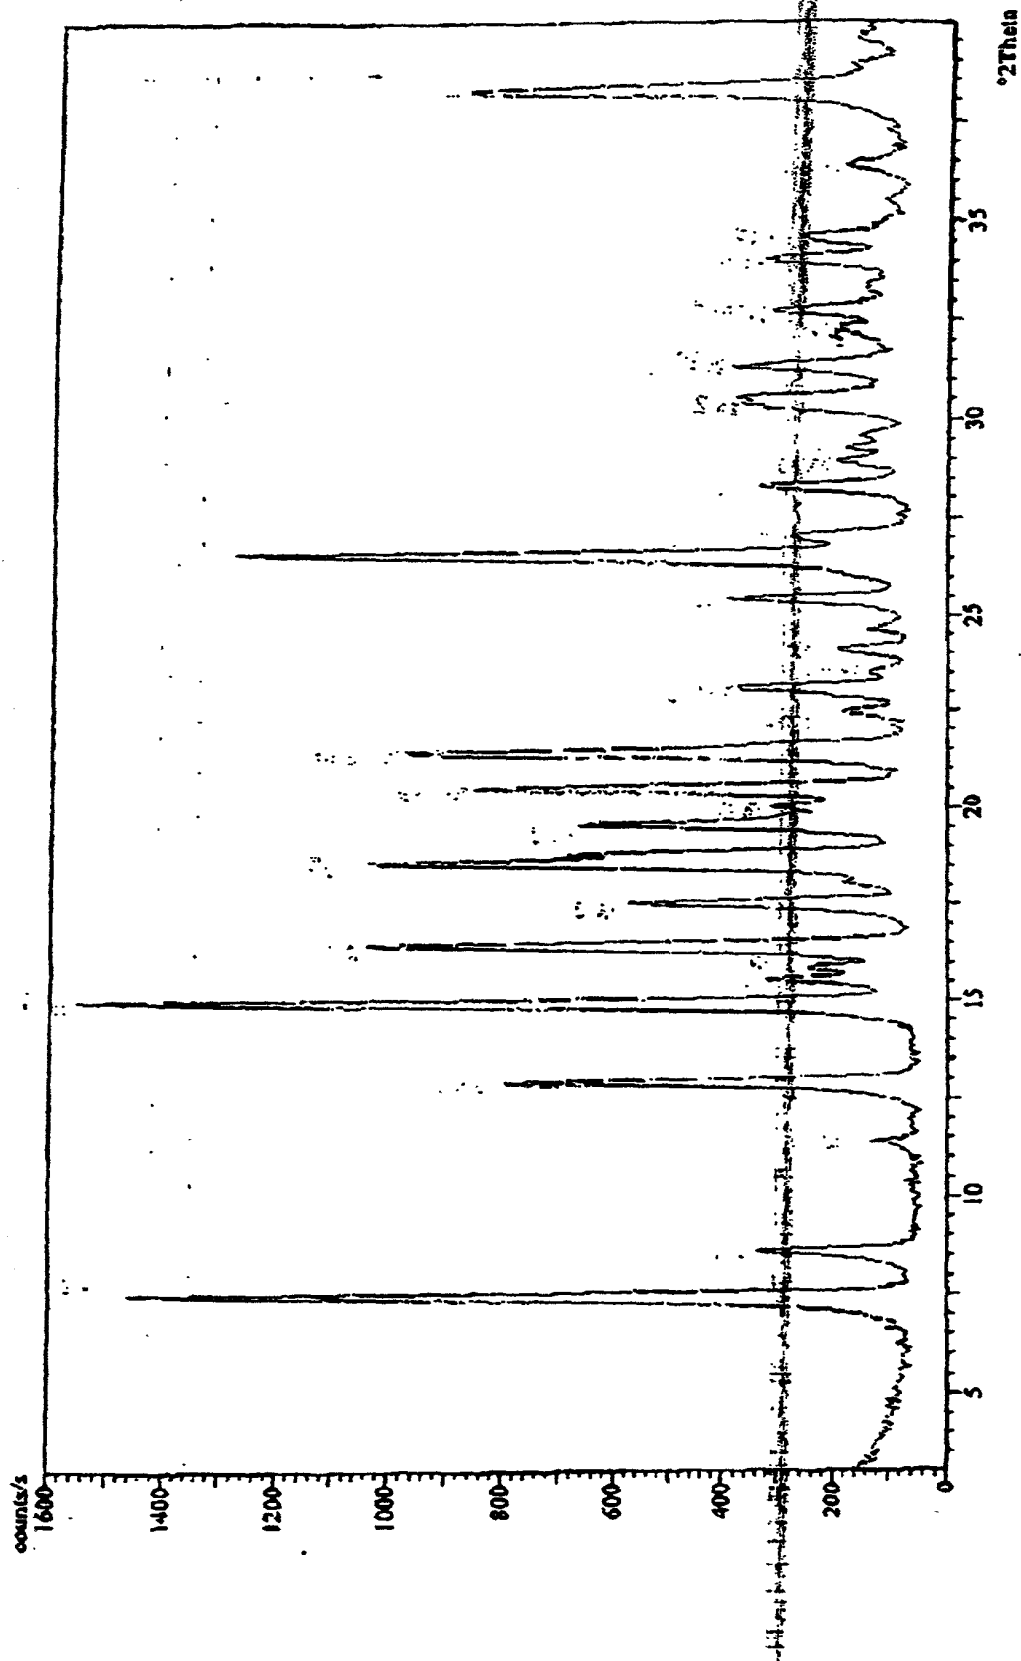


Figure 6

exo

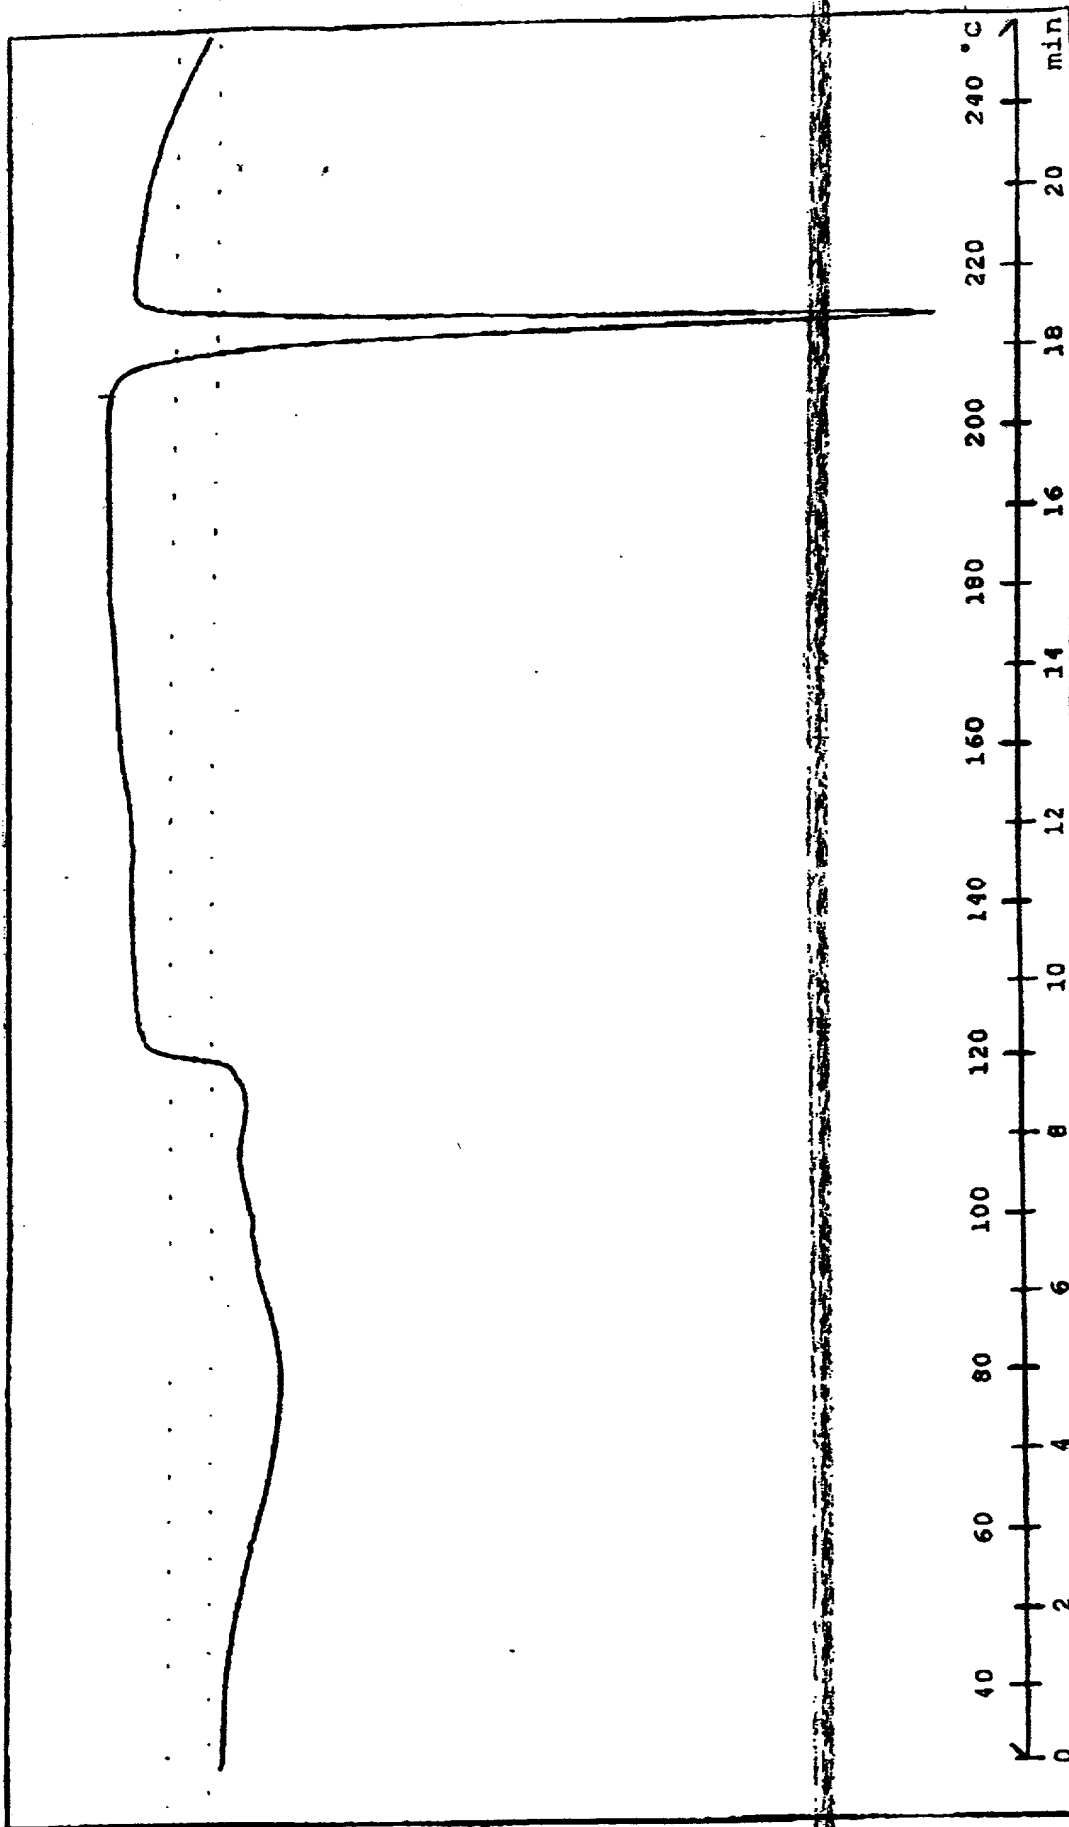

METTTLER TOLEDO STAR® System

Physical R&D Teva: Shlomo

Figure 7

TOTAL P.09

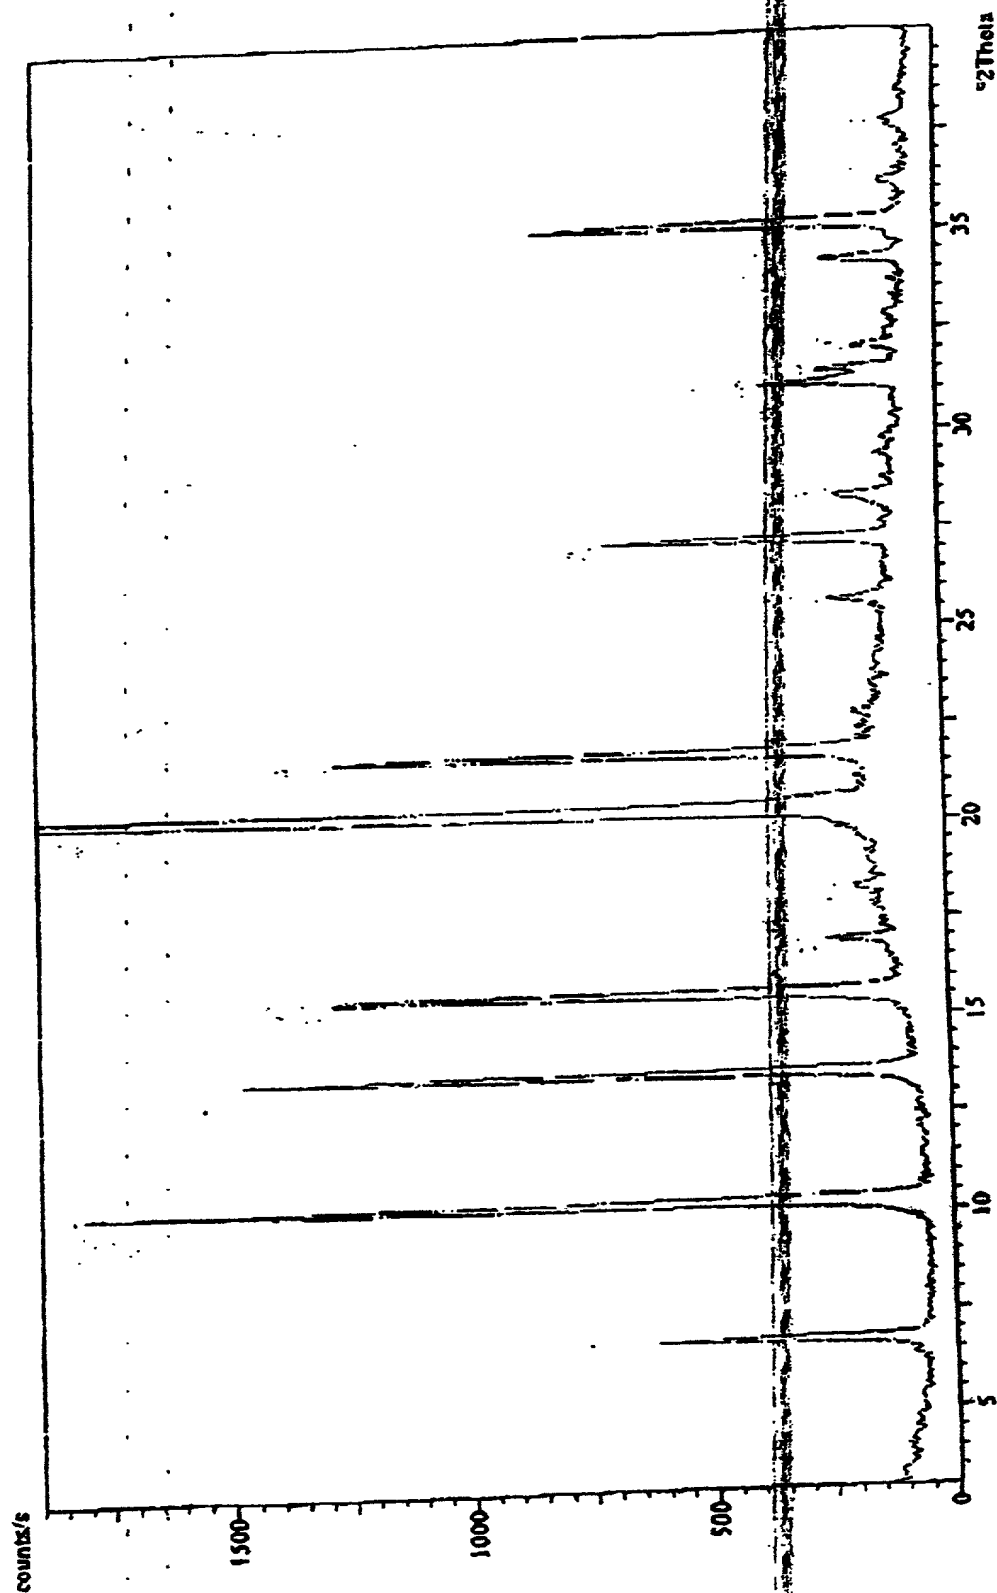


Figure 8



FILE: VEL-07 SHQ, ID: VEL-07 SHQ.

Date: 02/01/01 13:16 Step: 0.050° Cnt Time: 1.000 Sec.

Range: 2.00 - 40.00 (Deg) Cont. Scan Rate: 3.00 Deg/min. TSV

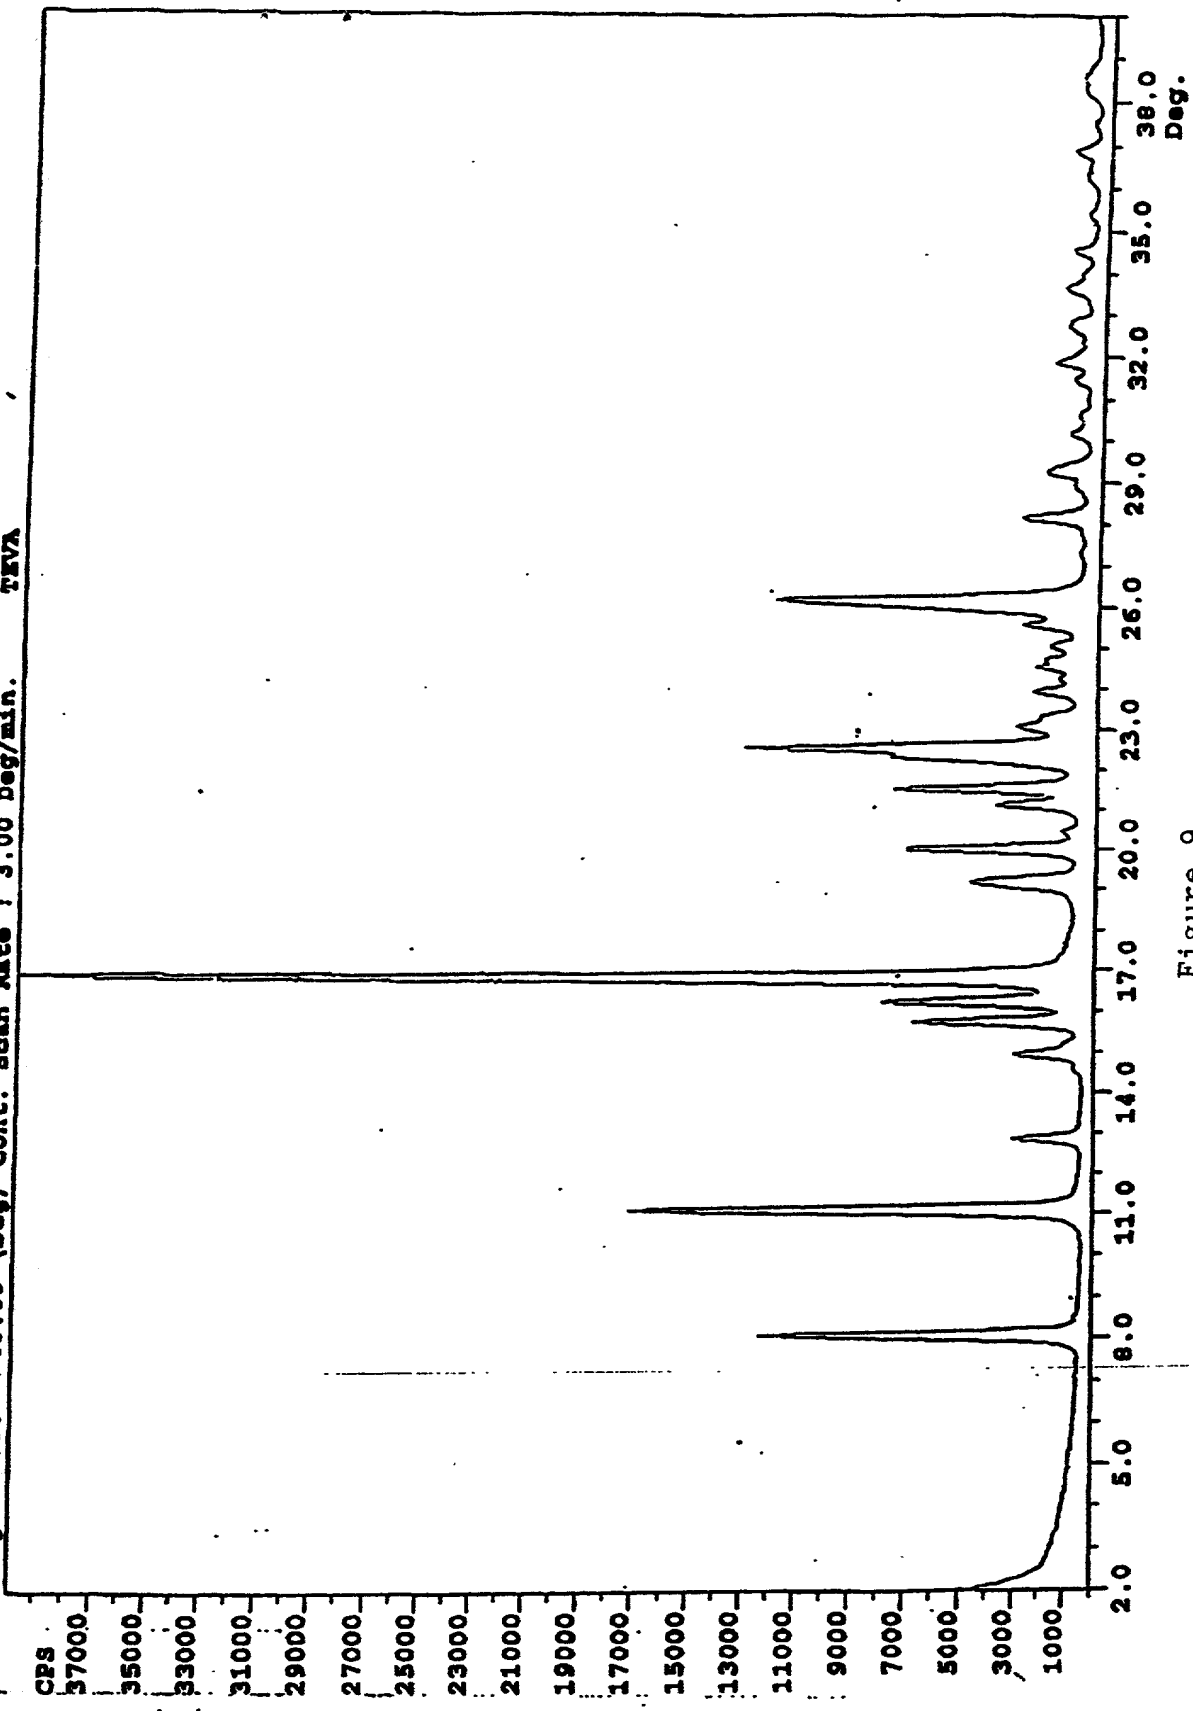


Figure 9

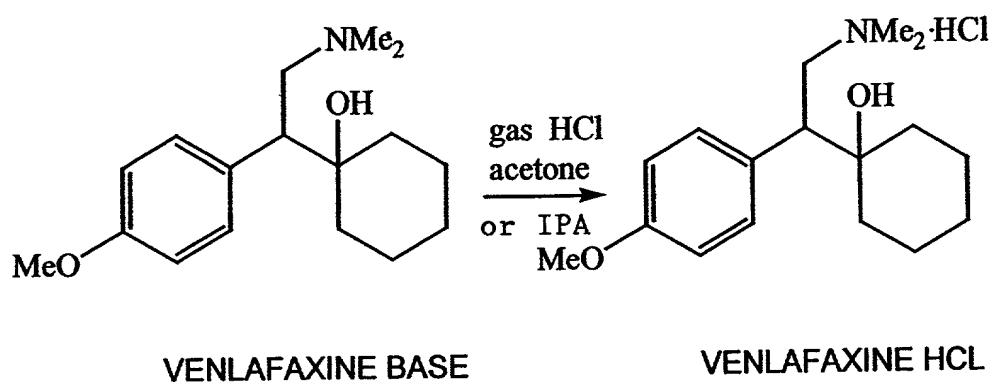


FIGURE 10